

(19)



Europäisches Patentamt

European Patent Office

Office européen des brevets



(11)

EP 1 145 177 B1

(12)

EUROPEAN PATENT SPECIFICATION

(45) Date of publication and mention
of the grant of the patent:
20.10.2004 Bulletin 2004/43

(21) Application number: **00913502.1**

(22) Date of filing: **17.02.2000**

(51) Int Cl.7: **G06F 19/00**

(86) International application number:
PCT/US2000/004079

(87) International publication number:
WO 2000/051055 (31.08.2000 Gazette 2000/35)

(54) **METHOD AND APPARATUS FOR MONITORING THERAPY EFFECTIVENESS**

VERFAHREN UND VORRICHTUNG ZUR BEOBACHTUNG DER THERAPIEEFFEKTIVITÄT

PROCEDE ET DISPOSITIF DE SURVEILLANCE DE L'EFFICACITE D'UNE THERAPIE AU MOYEN
D'UNE TECHNIQUE DE CONVERGENCE EXPONENTIELLE EXECUTEE A L'AIDE DE MESURES
DE CHARGE VIRALE D'APRES UN JEU ORDONNE DE MICRO-DEPOTS D'ADN

(84) Designated Contracting States:
**AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE**

(30) Priority: **22.02.1999 US 253791**

(43) Date of publication of application:
17.10.2001 Bulletin 2001/42

(60) Divisional application:
03028719.7 / 1 406 199

(73) Proprietor: **Vialogy Corporation**
Altadena, CA 91011 (US)

(72) Inventor: **GULATI, Sandeep**
La Canada, CA 91011 (US)

(74) Representative: **Schmidt, Steffen J., Dipl.-Ing.**
Wuesthoff & Wuesthoff,
Patent- und Rechtsanwälte,
Schweigerstrasse 2
81541 München (DE)

(56) References cited:

EP-A- 0 854 197
WO-A-98/07888
US-A- 5 389 512

WO-A-93/21339
WO-A-99/66024

- **HARRIS F ET AL: "ADAPTIVE FILTERS USING FRACTAL DIMENSION OF DATA" PROCEEDINGS OF THE ASILOMAR CONFERENCE ON SIGNALS, SYSTEMS AND COMPUTERS,US,NEW YORK, IEEE, vol. CONF. 24, 5 November 1990 (1990-11-05), pages 278-282, XP000280030**
- **PETER J. DAILEY AND DAMIAN HAYDEN: "Viral Load Assays: Methodologies, Variables, and Interpretation" THE AIDS KNOWLEDGE BASE, [Online] April 1998 (1998-04), XP002149413 Retrieved from the Internet: <URL:http://hivinsite.ucsf.edu/akb/current/02qrna/index.html> [retrieved on 2000-10-05]**

Remarks:

WIPO A3 publication data is not currently available.

Note: Within nine months from the publication of the mention of the grant of the European patent, any person may give notice to the European Patent Office of opposition to the European patent granted. Notice of opposition shall be filed in a written reasoned statement. It shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

EP 1 145 177 B1

Description**Field of the Invention**

- 5 **[0001]** The invention generally relates to techniques for monitoring the effectiveness of medical therapies and dosage formulations, and in particular to techniques for monitoring therapy effectiveness using viral load measurements.

Background of the Invention

- 10 **[0002]** It is often desirable to determine the effectiveness of therapies, such as those directed against viral infections, including therapies involving individual drugs, combinations of drugs, or other related therapies. One conventional technique for monitoring the effectiveness of a viral infection therapy is to measure and track a viral load associated with the viral infection, wherein the viral load is a measurement of a number of copies of the virus within a given quantity of blood, such per milliliter of blood. The therapy is deemed effective if the viral load is decreased as a result of the
- 15 therapy. A determination of whether any particular therapy is effective is helpful in determining the appropriate therapy for a particular patient and also for determining whether a particular therapy is effective for an entire class of patients. The latter is typically necessary in order to obtain FDA approval of any new drug or medical device therapy. Viral load monitoring is also useful for research purposes such as for assessing the effectiveness of new antiviral compounds determine, for example, whether it is useful to continue developing particular antiviral compounds or to attempt to gain
- 20 FDA market approval.
- [0003]** A test to determine the viral load can be done with blood drawn from T-cells or from other standard sources. The viral load is typically reported either as an absolute number, i.e., the number of virus particles per milliliter of blood or on a logarithmic scale. Likewise, decreases in viral load are reported in absolute numbers, logarithmic scales, or as percentages.
- 25 **[0004]** It should be noted though that a viral load captures only a fraction of the total virus in the body of the patient, i.e., it tracks only the quantity of circulating virus. However, viral load is an important clinical marker because the quantity of circulating virus is the most important factor in determining disease outcome, as changes in the viral load occur prior to changes in other detectable factors, such as CD4 levels. Indeed, a measurement of the viral load is rapidly becoming the acceptable method for predicting clinical progression of certain diseases such as HIV.
- 30 **[0005]** Insofar as HIV is concerned, HIV-progression studies have indicated a significant correlation between the risk of acquiring AIDS and an initial HIV baseline viral load level. In addition to predicting the risk of disease progression, viral load testing is useful in predicting the risk of transmission. In this regard, infected individuals with higher viral load are more likely to transmit the virus than others.
- [0006]** Currently, there are several different systems for monitoring viral load including quantitative polymerase chain reaction (PCR) and nucleic acid hybridization. Herein, the term viral load refers to any virological measurement using RNA, DNA, or p24 antigen in plasma. Note that viral RNA is a more sensitive marker than p24 antigen. p24 antigen has been shown to be detectable in less than 50% asymptomatic individuals. Moreover, levels of viral RNA rise and fall more rapidly than levels of CD4+ lymphocytes. Hence, changes in infection can be detected more quickly using viral load studies based upon viral RNA than using CD4 studies. Moreover, viral load values have to date proven to
- 35 be an earlier and better predictor of long term patient outcome than CD4-cell counts. Thus, viral load determinations are rapidly becoming an important decision aid for anti-retro viral therapy and disease management. Viral load studies, however, have not yet completely replaced CD4+ analysis in part because viral load only monitors the progress of the virus during infection whereas CD4+ analysis monitors the immune system directly. Nevertheless, even where CD4+ analysis is effective, viral load measurements can supplement information provided by the CD4 counts. For example,
- 40 an individual undergoing long term treatment may appear stable based upon the observation of clinical parameters and CD4 counts. However, the viral load of the patient may nevertheless be increasing. Hence, a measurement of the viral load can potentially assist a physician in determining whether to change therapy despite the appearance of long term stability based upon CD4 counts.
- [0007]** Thus, viral load measurements are very useful. However, there remains considerable room for improvement. One problem with current viral load measurements is that the threshold level for detection, i.e., the nadir of detection, is about 400-500 copies per milliliter. Hence, currently, if the viral load is below 400-500 copies per milliliter, the virus is undetectable. The virus may nevertheless remain within the body. Indeed, considerable quantities of the virus may remain within the lymph system. Accordingly, it would be desirable to provide an improved method for measuring viral load which permits viral load levels of less than 400-500 copies per milliliter to be reliably detected.
- 50 **[0008]** Another problem with current viral load measurement techniques is that the techniques are typically only effective for detecting exponential changes in viral loads. In other words, current techniques will only reliably detect circumstances wherein the viral load increases or decreases by an order of magnitude, such by a factor of 10. In other cases, viral load measurements only detect a difference between undetectable levels of the virus and detectable levels
- 55

of the virus. As can be appreciated, it would be highly desirable to provide an improved method for tracking changes in viral load which does not require an exponential change in the viral load for detection or which does not require a change from an undetectable level to a detectable level. Indeed, with current techniques, an exponential or sub-exponential change in the viral load results only in a linear change in the parameters used to measure the viral load. It would instead be highly desirable to provide a method for monitoring the viral load which converts a linear change in the viral load into an exponential change within the parameters being measured to thereby permit very slight variations in viral load to be reliably detected. In other words, current viral load detection techniques are useful only as a qualitative estimator, rather than as a quantitative estimator.

[0009] One reason that current viral load measurements do not reliably track small scale fluctuations in the actual number of viruses is that a significant uncertainty in the measurements often occurs. As a result, individual viral load measurements have little statistical significance and a relatively large number of measurements must be made before any statistically significant conclusions can be drawn. As can be appreciated it would be desirable to provide a viral load detection technique which can reliably measure the viral load such that the statistical error associated with a single viral load measurement is relatively low to permit individual viral load measurements to be more effectively exploited.

[0010] Moreover, because individual viral load measurements are not particularly significant when using current methods, treatment decisions for individual patients based upon the viral load measurements must be based only upon long term changes or trends in the viral load resulting in a delay in any decision to change therapy. It would be highly desirable to provide an improved method for measuring and tracking viral load such that treatment decisions can be made much more quickly based upon short term trends of measured viral loads.

[0011] As noted above, the current nadir of viral load detectability is at 400-500 copies of the virus per milliliter. Anything below that level is deemed to be undetectable. Currently the most successful and potent multi-drug therapies are able to suppress viral load below that level of detection in about 80-90 percent of patients. Thereafter, viral load is no longer an effective indicator of therapy. By providing a viral load monitoring technique which reduces the nadir of detectability significantly, the relative effectiveness of different multi-drug therapies can be more effectively compared. Indeed, new FDA guidelines for providing accelerated approval of a new drug containing regimen requires that the regimen suppress the viral load below the current nadir of detection in about 80 to 85 percent of cases. If the new regimen suppresses the viral load to undetectable levels in less than 80 to 85 percent of the cases, the new drug will gain accelerated approval only if it has other redeeming qualities such as a preferable dosing regimen (such as only once or twice per day), a favorable side effect profile, or a favorable resistance or cross-resistance profile. Thus, the ability of a regimen to suppress the viral load below the level of detection is an important factor in FDA approval. However, because the level of detectability remains relatively high, full approval is currently not granted by the FDA solely based upon the ability of the regimen to suppress the viral load below the minimum level of detection. Rather, for full approval, the FDA may require a further demonstration of the durability of the regimen, i.e., a demonstration that the drug regimen suppresses the viral load below the level of detectability and keeps it below the level of detectability for some period of time.

[0012] As can be appreciated, if a new viral load measurement and tracking technique were developed which could reliably detect viral load at levels much lower than the current nadir of detectability, the FDA may be able, using the new technique, to much more precisely determine the effectiveness of a drug regimen for the purposes of granting approval such that a demonstration of the redeeming qualities will no longer be necessary.

[0013] For all of these reasons, it would be highly desirable to provide an improved technique for measuring and tracking viral load capable of providing much more precise and reliable estimates of the viral load and in particular capable of reducing the nadir of detectability significantly. The present invention is directed to this end.

Summary of the Invention

[0014] In accordance with the invention, a method according to claim 1 is provided for determining the effectiveness of a therapy, such as an anti-viral therapy, by analyzing microarray output patterns generated from biological samples taken at different sampling times from a patient undergoing the therapy. In accordance with the method, a viral diffusion curve associated with a therapy of interest is generated and each of the output patterns representative of hybridization activity is then mapped to coordinates on the viral diffusion curve using fractal filtering. A degree of convergence between the mapped coordinates on the viral diffusion curve is determined. Then, a determination is made as to whether the therapy of interest has been effective based upon the degree of convergence.

[0015] In an exemplary embodiment, the viral diffusion curve is spatially parameterized such that samples map to coordinates near the curve maxima, if the viral load is increasing (i.e., therapy or dosage is ineffective). In this manner, any correlation between rate and extent of convergence across different patient samples is exploited to provide a quantitative and qualitative estimate of therapy effectiveness.

[0016] Also in the exemplary embodiment, the biological sample is a DNA sample. The output pattern of the microarray is quantized as a dot spectrogram. The viral diffusion curve is generated by inputting parameters representative

of viral load studies for the therapy of interest, generating a preliminary viral diffusion curve based upon the viral load studies; and then calibrating a degree of directional causality in the preliminary viral diffusion curve to yield the viral diffusion curve. The parameters representative of the viral load studies include one or more of baseline viral load (BVL) set point measurements at which detection is achieved, BVL at which therapy is recommended and viral load markers at which dosage therapy is recommended. The step of generating the preliminary viral diffusion curve is performed by selecting a canonical equation representative of the viral diffusion curve, determining expectation and mean response parameters for use in parameterizing the equation selected to represent the viral diffusion curve and parameterizing the equation selected to represent the viral diffusion curve to yield the preliminary viral diffusion curve.

[0017] Also, in the exemplary embodiment, each dot spectrogram is mapped to the viral diffusion curve using fractal filtering by generating a partitioned iterated fractal system IFS model representative of the dot spectrogram, determining affine parameters for IFS model, and then mapping the dot spectrogram onto the viral diffusion curve using the IFS. Before the dot spectrogram is mapped to the viral diffusion curve, the dot spectrogram is interferometrically enhanced. After the mapping, any uncertainty in the mapped coordinates is compensated for using non-linear information filtering.

[0018] Apparatus embodiment according to claim 16 is also provided. By exploiting aspects of the invention, disease management decisions related to disease progression, therapy and dosage effectiveness may be made by tracking the coordinates on the viral diffusion curve as successive DNA-/RNA-based microarray samples are collected and analyzed.

Brief Description of the Drawings

[0019] The features, objects, and advantages of the present invention will become more apparent from the detailed description set forth below when taken in conjunction with the drawings in which like reference characters identify correspondingly throughout and wherein:

FIG. 1 is a flow chart illustrating an exemplary method for determining the effectiveness of a viral therapy in accordance with the invention.

FIG. 2 is a flow chart illustrating an exemplary method for generating Viral Diffusion Curves for use with the method of Fig. 1.

FIG. 3 is a flow chart illustrating an exemplary method for mapping dot spectrograms onto Viral Diffusion Curves using fractal filtering for use with the method of Fig. 1.

FIG. 4 is a block diagram illustrating the effect of the fractal filtering of Fig. 3.

FIG. 5 is a flow chart illustrating an exemplary method for compensating for uncertainty using non-linear information filtering for use with the method of Fig. 1.

Detailed Description of Exemplary Embodiments

[0020] With reference to the figures, exemplary method embodiments of invention will now be described. The exemplary method will be described primarily with respect to the determination of changes in viral loads based upon the output patterns of a hybridized biochip microarray using DNA samples, but principles of the invention may be applied to other protein-based samples or to other types of output patterns as well.

[0021] With reference to FIG. 1, steps will be described for generating viral diffusion curves for use in processing DNA biomicroarray output patterns to determine the effectiveness of therapies imposed upon a patient providing samples for which the outputs are generated. Then, steps will be described for processing the specific output patterns using the VDC's.

[0022] An underlying clinical hypothesis of the exemplary method is that antiviral treatment should inhibit viral replication and lower an individual's viral load from baseline or suppress rising values. A stationary or rising viral load after the introduction of antiviral therapy indicates a lack of response to the drug(s) or the development of drug resistance. The VDC exploits the underlying hypothesis in part by correlating the rate of disease progression to a sample point value such that a change in sample point indicates progression.

The Method

[0023] At step 100, parameters representative of viral load studies for the therapy of interest are input. A preliminary viral diffusion curve is generated, at step 102, based upon the viral load studies. The parameters representative of the viral load studies include baseline viral load (BVL) set point measurements at which detection is achieved, BVL at which therapy is recommended and viral load markers at which dosage therapy is recommended. At step 104, a degree of directional causality in the preliminary viral diffusion curve is calibrated to yield the final viral diffusion curve.

EP 1 145 177 B1

[0024] Steps 100 - 104 are performed off-line for setting up the VDC's. These steps need be performed only once for a given therapy and for a given set of baseline viral load measurements. Thereafter, any number of DNA biomicroarray output patterns may be processed using the VDC's to determine the effectiveness of the therapy. Preferably, VDC's are generated for an entire set of therapies that may be of interest such that, for any new DNA biomicroarray output pattern, the effectiveness of any of the therapies can be quickly determined using the set of VDC's. In general, the aforementioned steps need be repeated only to update the VDC's based upon new and different baseline viral load studies or if new therapies of interest need to be considered.

[0025] In the following, steps will be summarized for processing DNA biomicroarray output patterns using the VDC's to determine whether any therapies of interest represented by the VDC's are effective. To determine the effectiveness of therapy at least two samples of DNA to be analyzed are collected from a patient, preferably taken some time apart, and biomicroarray patterns are generated therefrom. In other cases though, the different samples are collected from different patients.

[0026] The output patterns for the DNA biomicroarray are referred to herein as dot spectrograms. A dot spectrogram is generated using a DNA biomicroarray for each sample from an N by M DNA biomicroarray. An element of the array is an "oxel": $o(i,j)$. An element of the dot spectrogram is a "hixel": $h(i,j)$. The dot spectrogram is represented by cell amplitudes given by $\Phi(i,j)$ for i : 1 to N, and j : 1 to M.

[0027] Dot spectrograms are generated from the samples taken at different times using a prefabricated DNA biomicroarray at step 106. The dot spectrograms are interferometrically enhanced at step 108. Each dot spectrogram is then mapped to coordinates on the viral diffusion curves using fractal filtering at step 110. After the mapping, any uncertainty in the mapped coordinates is compensated for at step 112 using non-linear information filtering.

[0028] VDC coordinates are initialized at step 114, then updated in accordance with filtered dot spectrograms at step 116. A degree of convergence between the mapped coordinates on the viral diffusion curves is then determined at step 118 and a determination is made as to whether the therapy of interest has been effective. The determination is based upon whether the degree of convergence increases from one DNA sample to another. An increase in degree of convergence is representative of a lack of effectiveness of the therapy of interest. Hence, if the degree of convergence decreases, then execution proceeds to step 120, wherein a signal is output indicating that the therapy is effective. If the degree of convergence increases, then execution proceeds to step 122 wherein VDC temporal scale matching is performed. Then a determination is made at step 124 whether an effectiveness time scale has been exceeded. If exceeded, then a conclusion is drawn that the effectiveness of the viral therapy cannot be established even if more samples are analyzed. If not exceeded, then execution returns to step 106 wherein another sample taken from the same patient at a latter time is analyzed by repeating steps 106 through 118.

Viral Load Studies

[0029] Viral load studies for therapies of interest are parameterized at step 100 as follows. The therapy of interest is selected from a predetermined list of therapies for which viral load studies have been performed. Measurements from viral load studies are input for therapy of interest. As noted, the viral load measurements include one or more of Baseline Viral Load (BVL) set point measurements at which detection is achieved; BVL at which therapy is recommended; and VL markers at which dosage change recommended.

[0030] Data for the viral load measurements are obtained, for example, from drug qualification studies on a minimum include dosages, viral limits as well as time cycles within which an anti-viral drug is deemed effective. The data is typically qualified with age/weight outliers and patient history. Attribute relevant to this claim is the γ_1 or BVL_{LOW} which corresponds to the lowest detection limit shown for a therapy to be effective using conventional assays or any other diagnostic means. BVL_{NP-LOW} denotes the lowest threshold at which viral load is achieved using a nucleotide probe. Using interferometric enhancement technique, $BVL_{NP-LOW} < BVL_{LOW}$.

Generation of Viral Diffusion Curves

[0031] Referring now to FIG. 2, the viral diffusion curves are generated as follows. An equation is selected for representing the VDC at step 200. Expectation (μ) and mean response parameters are determined at step 202 for use in parameterizing the selected equation. Then the equation selected to represent the VDC is parameterized at step 204 to yield a numerical representation of the VDC. These steps will now be described in greater detail.

[0032] These steps populate a canonical machine representation, denoted as $VDC(i, \Gamma, \gamma, \kappa)$ (which is a special case of Fokker-Planck equation) to calibrate responses from a viral load detection DNA-array based hybridization biomicroarray.

i is the index for a diagnostic condition/therapy of interest,
 Γ denotes the parameter vector characterizing the VDC,

EP 1 145 177 B1

λ denotes the clinical endpoints vector that indicates detectability thresholds for a specific DNA-hybridization array implementation
 κ correspond to the uncertainty interval estimates.

5 [0033] An example of an equation selected for representing the VDC is:

$$\frac{\partial \rho}{\partial t} = \text{div}(\nabla \Psi(x) \rho) + \frac{\Delta \rho}{\beta}, \quad \rho(x, 0) = \rho^0(x)$$

10 [0034] The potential $\Psi(x): \mathcal{R}^n \rightarrow [0, \infty)$ is a smooth function, $\beta > 0$ is selected constant, and $\rho^0(x)$ is a probability density on \mathcal{R}^n .

[0035] Preferably, the diffusion potential of the equation and the BVL data are such that:

15
$$\Psi(x) < c \cdot [\text{BVL}_{\text{NP_LOW}} | \text{BVL}_{\text{LOW}}]$$

the constant c is generally set to

20
$$c = \frac{\text{[number of amplitude discretization levels]}}{[\log(\text{PCR amplification factor}) * \text{avg}(\text{oligonucleotides/oxel}) * \Gamma * \text{tagging efficiency} * \Gamma * \text{binding efficiency}]}$$

[0036] Binding efficiency is difficult to quantify analytically for a biomicroarray device technology. Hence, for use in the above equation, an estimate of the binding efficiency is preferably employed. A binding efficiency of 30% (.3) is appropriate, though other values may alternatively be used. Depending upon the specific biomicroarray used, the constant c typically ranges between 0.0001 to 0.5.

Expectation and Mean Response Parameters

30 [0037] The expectation (μ) and mean response parameters are then determined at step 202 for use in parameterizing the equation selected to represent the VDC. The expectation and mean response values are determined by: 1) performing conventional PCR amplification; 2) obtaining calibrated viral counts from the PCR amplification; 3) determining enhanced and normalized hybridization amplitude mean and variance values corresponding to the calibrated viral counts; and 4) matching the enhanced and normalized hybridization amplitude mean and variance values.

35 [0038] Two synthetic amplification techniques (in addition to PCR and any designer tagging) are used to achieve VL estimation above the BVL limit set for the exemplary embodiment of the method, namely (a) readout pre-conditioning, and (b) nonlinear interferometric enhancement. Moreover, the expectation match condition implies that:

40
$$\frac{\text{Expectation} [\text{Log}(\text{interferometrically enhanced image})]_{\text{V[expression set of interest]}}}{\text{Expectation} [\text{preconditioned image amplitude}]_{\text{V[expression set of interest]}}} \equiv 1$$

45 [0039] Variance matching is done similarly with respect to biomicroarray readout. The lower bound of mean response value can be given by:

50
$$\frac{\text{Variance} [\text{Log}(\text{interferometrically enhanced image})]_{\text{V[expression set of interest]}}}{\text{Variance} [\text{preconditioned image amplitude}]_{\text{V[expression set of interest]}}} \equiv 1$$

55 [0040] Using the above expression, a conservative lower bound for interferometric enhancement is estimated for each nucleotide expression of interest. Since the array fabrication device is assumed to have (i) an identical oligonucleotide density per oxel and (ii) equal length oligonucleotides, the same mean response amplitude can be assumed. If these two assumptions are not met then bounds need to be individually calculated and averaged using the above formula. Another assumption is that the binding efficiency is statistically independent of the actual oligonucleotide sequence. If this assumption does not hold for the specific device technology then the binding efficiency should be provided as well for each expressed sequence of interest. So the computational analysis method uses the analytically derived lower bounds, as computed using the above equation. This is a one-time calculation only and is done offline

at design time.

Parameterization of the VDC

- 5 [0041] The equation selected to represent the VDC is then parameterized using the expectation and mean response values at step 204 to yield a numerical representation of the VDC using

$$y(x) = \beta_0 + \beta_1 x + \beta_2 x^2$$

10

subject to constraints

15

$$\dot{x} = \gamma \sin \left[\frac{\sqrt{\omega}}{\alpha} (\beta_0 + \beta_1 x + \beta_2 x^2) \right] \sin \omega t + \varepsilon(t)$$

with constants α , β , γ and $\varepsilon \ll 1$.

20

[0042] This utility of this parameterization is established as follows. The VDC canonical representation is based on a variational formulation of the Fokker-Planck. The Fokker-Planck (FP) equation, or forward Kolmogorov equation, describes the evolution of the probability density for a stochastic process associated with an Ito stochastic differential equation. The exemplary method exploits the VDC to model a physical time-dependent phenomena in which randomness plays a major role. The specific variant used herein is one for which the drift term is given by the gradient of a potential. For a broad class of potentials (that correspond to statistical variability in therapy response), a time discrete, iterative variational is constructed whose solutions converge to the solution of the Fokker-Planck equation. The time-step is governed by the Wasserstein metric on probability measures. In this formulation the dynamics may be regarded as a gradient flux, or a steepest descent for the free energy with respect to the Wasserstein metric. This parameterization draws from theory of stochastic differential equations: wherein a (normalized) solution to a given Fokker-Planck equation represents the probability density for the position (or velocity) of a particle whose motion is described by a corresponding Ito stochastic differential equation (or Langevin equation). The drift coefficient is a gradient. The method exploits "designer conditions" on the drift and diffusion coefficients so that the stationary solution of a Fokker-Planck equation satisfies a variational principle. It minimizes a certain convex free energy functional over an appropriate admissible class of probability densities.

35

[0043] A physical analogy is to an optimal control problem which is related to the heating of a probe in a kiln. The goal is to control the heating process in such a way that the temperature inside the probe follows a certain desired temperature profile. The biomolecular analogy is to seek a certain property in the parameterized VDC—namely, an exponential jump in the VDC coordinate position for "small linear changes in the viral count".

40

[0044] This method is in contradistinction to conventional calibration strategies which obtain a linear or superlinear shift in quantization parameter for an exponential shift in actual viral count.

[0045] As noted, the form of FP equation chosen is :

$$\frac{\partial \rho}{\partial t} = \text{div}(\nabla \psi(x) \rho) + \frac{\Delta \rho}{\beta}, \quad \rho(x, 0) = \rho^0(x)$$

45

where the potential $\psi(x): \mathfrak{H}^n \rightarrow [0, \infty)$ is a smooth function, $\beta > 0$ is selected constant, and $\rho^0(x)$ is a probability density on \mathfrak{H}^n . The solution $\rho(t, x)$ is a probability density on \mathfrak{H}^n for almost every fixed time t . So the distribution $\rho(t, x) \geq 0$ for almost every $(t, x) \in (0, \infty) \times \mathfrak{H}^n$, and

50

$$\int_{\mathfrak{H}^n} \rho(t, x) dx = 1$$

for almost every $t, \in (0, \infty)$.

55

[0046] It is reasonably assumed that hybridization array device physics for the DNA biomicroarray (i.e., corresponding to the potential ψ) has an approximately linear response to the nucleotide concentration and the response is monotonic with bounded drift. So,

EP 1 145 177 B1

$$\rho_s(x) = \frac{1}{Z} e^{(-\beta \Psi(x))}$$

where the partition function Z is given by

$$Z = \int_{\mathcal{X}} e^{(-\beta \Psi(x))} dx$$

[0047] In this model the basis for device physics design is that the potential needs to be modulated such that it grows rapidly enough for Z to be finite. This is not achieved by conventional methods. However, a technique which does achieve this result is described in co-pending U.S. Patent Application xx/xxx,xxx, filed contemporaneously herewith, entitled "Method and Apparatus for Analyzing Hybridized DNA Microarray Patterns Using Resonant Interactions Employing Quantum Expressor Functions", which is incorporated by reference herein.

[0048] The probability measure $\rho_s(x)dx$ is the unique invariant measure for the Markov random field (MRF) fit to the empirical viral load data.

[0049] The method exploits a special dynamical effect to design p. The method restricts the FP equation form above to a more restricted case: random walk emulating between critical equilibrium points.

[0050] To aid in understanding this aspect of the invention, consider the diffusion form

$$\frac{\partial \rho(x,t)}{\partial t} = \frac{1}{2} D^2 \frac{\partial^2 \rho(x,t)}{\partial x^2}$$

where $D^2 = \pi \alpha^2$
and α is constant.

[0051] A specific VDC shape is parameterized by:

$$y(x) = \beta_0 + \beta_1 x + \beta_2 x^2$$

subject to constraints

$$\dot{x} = \gamma \sin \left[\frac{\sqrt{\omega}}{\alpha} (\beta_0 + \beta_1 x + \beta_2 x^2) \right] \sin \omega t + \varepsilon(t)$$

with constants α , β , γ and $\varepsilon \ll 1$.

[0052] These constants are set based upon the dynamic range expected for the viral load. Thus, if the viral load is expected to vary only within a factor of 10, the constants are set accordingly. If the viral load is expected to vary within a greater range, different constants are employed. The actual values of the constants also depend upon the particular disease.

[0053] Where the following conditions are met

$$\text{Expectation match: } E(x) = \int_{-\infty}^{\infty} x f(x) dx = \mu$$

$$\text{Variance: } \sigma^2 = \int_{-\infty}^{\infty} (x - \mu)^2 f(x) dx$$

And

$$\int_{-\infty}^{\infty} f(x) = 1$$

[0054] The expectation and mean response parameters for use in these equations are derived, as described above, from matching the enhanced and normalized hybridization amplitude mean and variance that correspond to calibrated viral counts (via classical PCR amplification).

[0055] A distribution represented by the above-equations then satisfies the following form with a prescribed probability distribution

$$\dot{x} = \gamma \sin \left[\frac{\sqrt{\omega}}{\alpha} y(x) \right] \sin \omega t + \varepsilon(t)$$

[0056] Assuming:

$$y' = \frac{dy}{dx} > \beta > 0, \beta = \text{constant}$$

and

$$\varepsilon(t) = \varepsilon_0 a y$$

such that

$$\dot{a} = a^{1/3} (y - 1)(y + 1) - \varepsilon_0 a$$

and the distribution controlling equation is

$$f(x) = 0.5 |y'(x)|$$

such that $y(-1) < x < y(1)$.

[0057] The characteristic timescale of response for this system is given by

$$T^* = \frac{1}{\omega} \arccos \left[1 - \frac{B(1/3, 1/3)}{\sqrt[3]{2}} \frac{\alpha \sqrt{\omega}}{\gamma} \right]$$

the successive points must show a motion with characteristic timescale. The VDC is designed such that sampling time falls well within characteristic time.

[0058] As noted the actual information used for populating above the parameters is available from the following: Baseline viral load (BVL) set point measurements at which detection is achieved; BVL at which therapy is recommended; and VL markers at which dosage change recommended.

[0059] The following provides an example of preclinical data that is available to assist in parameterizing the VDC.

EP 1 145 177 B1

NOTIONAL VIRAL LOAD MANAGEMENT EXAMPLE

[0060] This is a synthetic example to illustrate how data from clinical studies may be used to calibrate the VDC.

5 [0061] Viral Load analysis studies, using conventional assays, in HIV progression have shown that neither gender, age, HCV co-infection, past history of symptomatic HIV-1 infection, duration of HIV-1 infection nor risk group are associated with a higher risk of increasing baseline viral load (BVL) to the virologic end-point. However, patients with a high (BVL) between 400-6000 copies had a 10-fold higher risk of increasing the level of viral load than patients with a BVL below 1500 copies/ml. Thus, baseline viral load set point measurements provide an important indicator for onset of disease.

10 [0062] Initiation of antiretroviral therapy is generally recommended when the CD4⁺ T-cell count is < 600 cells/mL and the viral load level is > 6,000 copies/mL. When the viral load is > 28000 copies/mL, initiation of therapy is recommended regardless of other laboratory markers and clinical status.

[0063] Effective antiretroviral treatment may be measured by changes in plasma HIV RNA levels. The ideal end point for effective antiviral therapy is to achieve undetectable levels of virus (< 400 copies/mL). A decrease in HIV RNA levels of at least 0.5 log suggests effective treatment, while a return to pretreatment values (± 0.5 log) suggests failure of drug treatment.

[0064] When HIV RNA levels decline initially but return to pretreatment levels, the loss of therapy effectiveness has been associated with the presence of drug-resistant HIV strains.

20 [0065] The therapy-specific preclinical viral load markers (such as low and high limits in the above example) are used to establish actual BVL boundaries for the VDC associated with a particular therapy. In this regard, the determination of the BVL parameters is disease specific. For example, in HIV methods such as RT-PCR, bDNA or NASBA are used. Other diseases use other assays. Typically, once the parameters of the VDC equation have been set (i.e. constants α , β , γ and ϵ), only two viral load markers are needed to complete the parameterization of the VDC. This is in contrast to previous techniques whereby expensive and laborious techniques are required to determine the shape of a viral diffusion curve. The present invention succeeds in using only two viral load markers in most cases by exploiting the canonical VDC described above which has predefined properties and which is predetermined based upon the particular biochip being used.

30 Calibration of Viral Diffusion Curves

[0066] Referring again to FIG. 1, the directional causality of the VDC is calibrated at step 104 in the context of an NIF discussed in greater detail below. At least arbitrarily selected three sample points are used execute the NIF calibration computation. The resulting polynomial is used to extracting qualitative coherence properties of the system.

35 [0067] The spectral $[\Theta]$ and temporal coherence $[\vartheta]$ is incrementally estimated and computed for each mutation/oligonucleotide of interest by a NIF forward estimation computation (described further below). The two estimates are normalized and convolved to yield cross-correlation function over time. The shape index (i.e., curvature) of the minima is used as a measure for directional causality. Absence of curvature divergence is used to detect high directional causality in the system.

40 Sample Collection

[0068] Samples are collected at step 106 subject to a sample point collection separation amount. The separation amount for two samples is preferably within half a "drug effectiveness mean time" covering 2σ population level wherein σ denotes the standard deviation in period before which a effectiveness for a particular drug is indicated. The following are some general guidelines for sample preparation for use with the exemplary method:

- It is important that assay specimen requirements be strictly followed to avoid degradation of viral RNA.
- A baseline should be established for each patient with two specimens drawn two to four weeks apart.
- Patients should be monitored periodically, every three to four months or more frequently if therapy is changed. A viral load level that remains at baseline or a rising level indicates a need for change in therapy.
- Too much significance should not be given to any one viral load result. Only sustained increases or decreases of 0.001- 0.01 log [conventional methods typically require a 0.3-0.5 log change] or more should be considered significant. Biological and technical variation of up to 0.01 log [typical conventional limit: 0.3 log] is possible. Also, recent immunization, opportunistic infections and other conditions may cause transient increases in viral load levels.
- A new baseline for each patient should be established when changing laboratories or methods.

[0069] Recommendations for frequency of testing are as follows:

EP 1 145 177 B1

- establish baseline: 2 measurements, 2 to 4 weeks apart
- every 3 to 4 months or in conjunction with CD4⁺ T-cell counts
- 3 to 4 weeks after initiating or changing antiretroviral therapy
- shorter intervals as critical decisions are made.
- 5 - measurements 2-3 weeks apart to determine a baseline measurement.
- repeat every 3-6 months thereafter in conjunction with CD4 counts to monitor viral load and T-cell count.
- avoid viral load measurements for 3-4 weeks following an immunization or within one month of an infection.
- a new baseline for each patient should be established when changing laboratories or methods.

10 **[0070]** The samples are applied to a prefabricated DNA biomicroarray to generate one or more dot spectrograms each denoted $\Phi(i,j)$ for $i: 1$ to N , and $j: 1$ to M . The first sample is referred to herein as the $k=1$ sample, the second as the $k=2$ sample, and so on.

Interferometric Enhancement of the Dot Spectrogram

15 **[0071]** Each dot spectrogram provided by the DNA biomicroarray is filtered at step 108 to yield enhanced dot spectrograms $\Phi(x)$ either by performing a conventional Nucleic Assay Amplification or by applying preconditioning and normalization steps as described in the co-pending Patent Application having Serial Number 09/253,789, entitled "Method And Apparatus For Analyzing Hybridized Biochip Patterns Using Resonance Interactions Employing Quantum Expressor Functions". The application is incorporated by reference herein, particularly insofar as the descriptions of the use of preconditioning and normalization curves are concerned.

Fractal Filtering

25 **[0072]** Each enhanced dot spectrogram is then mapped to the VDC using fractal filtering at step 110 as shown in FIG. 3 by generating a partitioned iterated fractal system 302, determining affine parameters for the IFS 304 and then mapping the enhanced dot spectrogram onto the VDC using the IFS, step 306.

[0073] The VDC representation models a stochastic process given by

$$W(f)(x,y) = \begin{cases} \gamma_i \cdot f \left(\frac{1}{\sigma_i} \left(\frac{x-x'_D}{y-y'_D} \right) + \frac{x'_R}{y'_R} \right) + \tau \left(\frac{x-x'_D}{y-y'_D} \right) + \beta_i, \\ \text{if } (x,y) \in \mu_i^{-1}(1), \text{ for some } 1 \leq i \leq m; \\ \\ 0, & \text{otherwise;} \end{cases}$$

for any $(x,y) \in \mathbb{R}^2$ and $f \in \mathcal{F}(\mathbb{R}^2)$

45 **[0074]** An exemplary partitioned iterated fractal system (IFS) model for the system is

$$W = \{\Phi_i = (\mu_i, T_i)\} i = 1, 2, \dots, m$$

50 where the affine parameters for the IFS transformation are given by

$$T_i = \left((x'_D, y'_D), (x'_R, y'_R), \sigma_i = \begin{pmatrix} s_{00} & s_{01} \\ s_{10} & s_{11} \end{pmatrix}, \tau_i = (t'_0, t'_1), \gamma_i, \beta_i \right)$$

where the D - origin is given by (x'_D, y'_D) .

the R -origin is given by (x_R^i, y_R^i)
 spatial transformation matrix is given by σ_i
 the intensity tilting vector is given by τ_i
 the contrast adjustment is given by γ_i ,
 the brightness adjustment is given by β_i ,
 and wherein Φ represents the enhanced dot spectrogram and wherein μ represents the calculated expectation
 match values

[0075] This IFS model maps the dot spectrogram to a point on the VDC wherein each VDC coordinate is denoted
 by $VDC(t, \Theta)$ such that

$$W[\Phi, k] \rightarrow VDC(k, \Theta)$$

Wherein k represents a sample.

[0076] In the above equation, Θ represent the parameters of the IFS map.

[0077] Thus the output of step 110, is a set of VDC coordinates, identified as $VDC(k, \Theta)$, with one set of coordinates
 for each enhanced dot spectrogram $k = 1, 2, \dots, n$.

[0078] The effect of the steps of FIG. 3 is illustrated in FIG. 4 which shows a set of dot spectrograms 450, 451 and
 452 and a VDC 454. As illustrated, each dot spectrogram is mapped to a point on the VDC. Convergence toward a
 single point on the VDC implies ineffectiveness of the viral therapy. A convergence test is described below.

Uncertainty Compensation

[0079] With reference to FIG. 5, any uncertainty in the coordinates $VDC(k, \Theta)$ is compensated using Non-linear
 Information Filtering as follows. Biomicroarray dispersion coefficients, hybridization process variability values and em-
 pirical variance are determined at step 402. The biomicroarray dispersion coefficients, hybridization process variability
 values and empirical variance are then converted at step 404 to parameters for use in NIF. The NIF is then applied at
 step 406 to the VDC coordinates generated at step 106 of FIG. 1.

[0080] Nonlinear information filter (NIF), is a nonlinear variant of the *Extended Kalman Filter*. A nonlinear system is
 considered. Linearizing the state and observation equations, a linear estimator which keeps track of total state estimates
 is provided. The linearized parameters and filter equations are expressed in information space. This gives a filter that
 predicts and estimates information about *nonlinear* state parameters given nonlinear observations and nonlinear sys-
 tem dynamics.

[0081] The information Filter (IF) is essentially a Kalman Filter expressed in terms of measures of the amount of
 about the parameter of interest instead of tracking the states themselves, i.e., track the inverse covariance form of the
 Kalman filter. Information here is in the *Fisher* sense, i.e. a measure of the amount of information about a parameter
 present in the observations.

[0082] Uncertainty bars are estimated using NIF algorithm. The parameters depend on biomicroarray dispersion
 coefficients, hybridization process variability and empirical variance indicated in the trial studies.

[0083] One particular advantage of the method of the invention is that it can also be used to capture the dispersion
 from individual to individual, therapy to therapy etc. It is extremely useful and enabling to the method in that it can be
 apriori analytically set to a prechosen value and can be used to control the quality of biomicroarray output mapping to
 VDC coordinates.

[0084] The biomicroarray dispersion coefficients, hybridization process variability values and empirical variance are
 determined as follows. Palm generator functions are used to capture stochastic variability in hybridization binding
 efficacy. This method draws upon results in stochastic integral geometry and geometric probability theory.

[0085] Geometric measures are constructed to estimate and bound the amplitude wanderings to facilitate detection.
 In particular we seek a measure for each mutation-recognizer centered (MRC-) hixel that is invariant to local degra-
 dation. Measure which can be expressed by multiple integrals of the form

$$m(Z) = \int f(z) dz$$

where Z denotes the set of mutations of interest. In other words, we determine the function $f(z)$ under the condition
 that $m(z)$ should be invariant with respect to all dispersions ξ . Also, up to a constant factor, this measure is the only
 one which is invariant under a group of motions in a plane. In principle, we derive deterministic analytical transformations

EP 1 145 177 B1

on each MRC-hixel., that map error-elliptic dispersion bound defined on \mathfrak{R}^2 (the two dimension Euclidean space - i.e., oxel layout) onto measures defined on \mathfrak{R} . The dispersion bound is given by

$$\text{Log}_4(\hat{O}_{(i,j)}|^2).$$

[0086] Such a representation of uniqueness facilitates the rapid decimation of the search space. It is implemented using a filter constructed using measure-theoretic arguments. The transformation under consideration has its theoretical basis in the Palm Distribution Theory for point processes in Euclidean spaces, as well as in a new treatment in the problem of probabilistic description of MRC-hixel dispersion generated by a geometrical processes. Latter is reduced to a calculation of intensities of point processes. Recall that a point process in some product space $E \times F$ is a collection of random realizations of that space represented as $\{(e_i, f_i), | e_i \in E, f_i \in F\}$.

[0087] The Palm distribution, Π of a translation (T_n) invariant, finite intensity point process in \mathfrak{R}^* is defined to the conditional distribution of the process. Its importance is rooted in the fact that it provides a complete probabilistic description of a geometrical process.

[0088] In the general form, the Palm distribution can be expressed in terms of a Lebesgue factorization of the form

$$E_P N^* = \Lambda \cdot L_N \times \Pi$$

[0089] Where Π and Λ completely and uniquely determine the source distribution P of the translation invariant point process. Also, $E_P N^*$ denotes the first moment measure of the point process and L_N is a probability measure.

[0090] Thus a determination of Π and Λ is needed which can uniquely encode the dispersion and amplitude wandering associated with the MRC-hixel. This is achieved by solving a set of equations involving Palm Distribution for each hybridization (i.e., mutation of interest). Each hybridization is treated as a manifestation of a stochastic point process in \mathfrak{R}^*

[0091] In order to determine Π and Λ we have implemented the following measure-theoretic filter:

Determination of Λ

using integral formulae constructed using the marginal density functions for the point spread associated with MRC-hixel (i,j)

The oligonucleotide density per oxel $\rho_{m(i,j)}$, PCR amplification protocol (σ_m) , fluorescence binding efficiency (η_m) and imaging performance $(\bar{\omega}_m)$ provide the continuous probability density function for amplitude wandering in the m -th MRC-hixel of interest. Let this distribution be given by $(\rho_{m(i,j)}, \sigma_m, \eta_m, \bar{\omega}_m)$.

- The method requires a preset binding dispersion limit to be provided to compute Λ . The second moment to the function

$$(\rho_{m(i,j)}, \sigma_m, \eta_m, \bar{\omega}_m)$$

at SNR = 0 condition is used to provide the bound.

Determination of Π

Obtained by solving the inverse problem

$$\Pi = \Theta^* P$$

where

$$P = \int_{\tau_1}^{\tau_2} \mathcal{P}(\rho_{m(i,j)}, \sigma_m, \eta_m, \bar{\omega}_m) d\tau$$

where τ_1 and τ_2 represent the normalized hybridization dispersion limits.

EP 1 145 177 B1

[0092] The number are empirically plugged in. The values of 0.1 and 0.7 are appropriate for, respectively, signifying loss of 10% - 70% hybridization. Also, Θ denotes the distribution of known point process. The form $1/(1+\exp(\varphi(\dots)))$ is employed herein to represent Θ .

[0093] The biomicroarray dispersion coefficients, hybridization process variability values and empirical variance are then converted to parameters at step 304 for use in NIF as follows.

[0094] The NIF is represented by:

$$\text{Predicted State} = f(\text{current state, observation model, information uncertainty, information model})$$

[0095] Detailed equations are given below.

[0096] In the biomicroarray context, NIF is an information-theoretic filter that predicts and estimates information about nonlinear state parameters (quality of observable) given nonlinear observations (e.g., post hybridization imaging) and nonlinear system dynamics (spatio-temporal hybridization degradation). The NIF is expressed in terms of measures of the amount of information about the observable (i.e., parameter of interest) instead of tracking the states themselves. It has been defined as the inverse covariance of the Kalman filter, where the information is in the Fisher sense, i.e, a measure of the amount of information about θ , present in the observations Z^k where the Fisher information matrix is the covariance of the score function.

[0097] In a classical sense the biomicroarray output samples can be described by the nonlinear discrete-time state transition equation of the form:

$$VDC(k) = f(VDC(k-1), \Phi(k-1), k) + v(k)$$

where $VDC(k-1)$ is the state at time instant $(k-1)$,
 $\Phi(k-1)$ is the input vector (embodied by dosage and/or therapy)
 $v(k)$ is some additive noise; corresponds to the biomicroarray dispersion as computed by the Palm Generator functions above.

$VDC(k)$ is the state at time k ,
 $f(k, \dots)$ is the nonlinear state transition function mapping previous state and current input to the current state. In this case it is the fractal mapping that provides the VDC coordinate at time k .

[0098] The observations of the state of the system are made according to a non-linear observation equation of the form

$$z(k) = h(VDC(k)) + w(k)$$

where $z(k)$ is the observation made at time k
 $VDC(k)$ is the state at time k ,
 $w(k)$ is some additive observation noise
and $h(\cdot, k)$ is the current non-linear observation model mapping current state to observations, i.e., sequence-by-hybridization made at time k ,

$v(k)$ and $w(k)$ are temporally uncorrelated and zero-mean. This is true for the biomicroarray in how protocol uncertainties, binding dynamics and hybridization degradation are unrelated and additive. The process and observation noises are uncorrelated.

$$E[v(i) w^T(j)] = 0, \quad \forall i, j.$$

[0099] The dispersion coefficients together define the nonlinear observation model.

[0100] The nonlinear information prediction equation is given by

$$\hat{y}(k|k-1) = Y(k|k-1) f(k, \hat{VDC}(k-1|k-1), u(k-1))$$

$$Y(k|k-1) = \left[\nabla f_x(k) Y^{-1}(k-1|k-1) \nabla f_x^T(k) + Q(k) \right]^{-1}$$

EP 1 145 177 B1

[0101] The nonlinear estimation equations are given by

$$\hat{y}(k|k) = \hat{y}(k|k-1) + i(k)$$

$$Y(k|k) = Y(k|k-1) + l(k)$$

where

$$l(k) = \nabla h_x^T(k) R^{-1}(k) \nabla h_x(k)$$

$$i(k) = \nabla h_x^T(k) R^{-1}(k) [v(k) + \nabla h_x(k) \hat{VDC}(k|k-1)]$$

where

$$v(k) = z(k) - h(\hat{x}(k|k-1))$$

[0102] In this method NIF helps to bind the variability in the VDC coordinate mapping across sample to sample so that dosage and therapy effectiveness can be accurately tracked.

[0103] The NIF is then applied to enhanced, fractal-filtered dot spectrogram at step 306 as follows. States being tracked correspond to post-hybridization dot spectrogram in this method. NIF computation as described above specifies the order interval estimate associated with a VDC point. It will explain and bound the variability in Viral load estimations for the same patient from laboratory to laboratory.

[0104] The NIF also specifies how accurate each VDC coordinate is given the observation model and nucleotide set being analyzed.

Convergence Testing

[0105] Referring again to FIG. 1, once any uncertainty is compensated, the VDC coordinates are renormalized at step 114. The renormalized VDC coordinates are patient specific and therapy specific. Alternately the coordinates could be virus / nucleotide marker specific. The NIF-compensated VDC coordinates are renormalized to the first diagnostic sample point obtained using the biomicroarray. Thus a patient can be referenced to any point on the VDC.

[0106] This renormalization step ensures that VDC properties are maintained, notwithstanding information uncertainties as indicated by the NIF correction terms. The approach is drawn from "renormalization-group" approach used for dealing with problems with many scales. In general the purpose of renormalization is to eliminate an energy scale, length scale or any other term that could produce an effective interaction with arbitrary coupling constants. The strategy is to tackle the problem in steps, one step for every length scale. In this method the renormalization methodology is abstracted and applied during a posteriori regularization to incorporate information uncertainty and sample-to-sample variations.

[0107] This is in contradistinction to current viral load measurement calibration methods that either generate samples with same protocol and same assumptions of uncertainty or use some constant correction term. Both existing approaches skew the viral load readout so that measurements are actually accurate only in a limited "information" and "observability" context. This explains the large variations in readings from different laboratories and technicians for the same patient sample.

[0108] Specifically, we include the dynamic NIF correction function to the gradient of the VDC at the sample point normalized in a manner such that when the information uncertainty is null, the correction term vanishes. As discussed in the above steps, the NIF correction terms is actually derived from the noise statistics of the microarray sample.

$$\langle VDC'(k, \Theta) \rangle = VDC(k, \Theta) + [\nabla NIF(Y, I)_k]$$

where $\nabla NIF(Y, I)_k$ denotes the gradient of nonlinear information prediction function. Under perfect observation model this term vanishes.

[0109] Once initialized, the VDC coordinates are then updated at step 116 applying the IFS filter $W[]$ on $k+1$ th sample,

EP 1 145 177 B1

by

VDC(k+1, Θ) ← W[Biomicroarray Output, K+1];

5

[0110] A direction convergence test is next performed at step 118 to determine whether the selected therapy has been effective. If convergence establishes that the viral load for the patient is moving in a direction representative of a lower viral load, then the therapy is deemed effective. The system is deemed to be converging toward a lower viral load if and only if:

10

$$\left\| \frac{VDC(t_k) - VDC(t_{k-j})}{VDC(t_{k-1}) - VDC(t_{k-j})} \right\| > 1 \wedge \left\| \frac{VDC_{peak} - VDC(t_k)}{VDC_{peak} - VDC(t_{k-1})} \right\| < 1 \text{ for } k > 2 \text{ and } j > 0$$

15

[0111] The above relationships needs to be monotonically persistent for at least two combinations of k and j.

[0112] Also, date[k] - date[j] < κ * characteristic time, \tilde{t} (in days)

20

[0113] Where κ captures the population variability. Typically, $\kappa < 1.2$.

[0114] The peak VDC value is determined based on the VDC. The peak amplitude is an artifact of the specific parameterization to the Fokker-Planck equation used in deriving the VDC. It is almost always derived independent of the specific sample.

25

[0115] In connection with step 118, a VDC Shift factor Δ may be specified at which a dosage effectiveness decision and/or disease progression decision can be made. The VDC shift factor is applied to estimate the VDC curvature traversed between two measurements.

30

[0116] If the system is deemed to be converging toward a lower viral load, an output signal is generated indicating that the therapy of interest is effective at step 120. If not, then the execution proceeds to step 122 wherein VDC scale matching is performed. A key assumption underlying this method is that movement along VDC is significant if and only if the sample points are with a constant multiple of temporal scale characterizing the VDC. This does not in any way preclude the pharmacological relevance associated with the datapoints. But complete pharmacological interpretation of the sample points is outside the scope of this method. The process is assumed to be cyclostationary or at a large time scale and two or more sample points have been mapped to VDC coordinates. The coordinates are then plugged into an analytic to estimate the empirical cycle time (\tilde{t}). This is implemented as described in the following sections.

35

[0117] Again the empirical cycle time (\tilde{t}) is used to establish decision convergence.

Scale Matching

40

[0118] Select a forcing function of the form:

$$= k \cdot \phi^m \cos \omega t$$

where k is a constant and m is a small odd integer ($m < 7$).

45

[0119] The phase space for this dynamical system is represented by:

50

$$\dot{x} = \gamma \sin \left[\frac{\sqrt{\omega}}{\alpha} \operatorname{erf} m \left(\frac{x}{\sigma \sqrt{2}} \right) \right]^{\frac{1}{k+2}} \sin \omega t$$

where

55

$$\operatorname{erf} m(x) = \begin{cases} -1 & \text{if } x < -N \\ \operatorname{erf}(x) & \text{if } |x| \leq N \\ 1 & \text{if } x > N \end{cases}$$

and $\operatorname{erf} m(\cdot)$ denotes the error function.

K is set to 1; where $0 < \alpha, \gamma, \omega < 1$ are refer to constants.

Let τ_{emp} denote the cycle-time-scale for this empirical system.

If $\log_e(\tau_{\text{emp}}/T) > 1$ (in step 10) then we claim that time-scales do not match.

Time Scale Testing

[0120] Next a determination has been made as to whether an effectiveness timescale has been exceeded at step 124 by:

Checking if a time step between successive sampling has exceeded T by determining if

$$\text{Time}_{k+1} - \text{Time}_k > T$$

such that $\text{VDC}(k+1, \Theta) - \text{VDC}(k, \Theta) < \zeta$ where
is set to 0.0001 and wherein
T is given by

$$T = \frac{1}{\omega} \arccos \left[1 - \frac{B(1/3, 1/3)}{\sqrt{2}} \frac{\alpha \sqrt{\omega}}{\gamma} \right]$$

$B(1/3, 1/3)$ represents the Beta function around the coordinates $(1/3, 1/3)$. We can actually use all $B(1/2+1, 1/2i+1)$ for $i > 1$ and $i < 7$.

If $\text{Time}_{k+1} - \text{Time}_k > T$ then output signal at step 126 indicating that either
no change in viral load concluded, OR
therapy deemed ineffective, OR
dosage deemed suboptimal.

[0121] If $\text{Time}_{k+1} - \text{Time}_k < T$ then process another sample by repeating all steps beginning with Step 4 wherein a dot spectrogram is generated for a new sample.

[0122] If the effectiveness time scale has been exceeded then a signal is output indicating that no determination can be as to whether the therapy of interest is effective. If the time scale is not exceeded, then execution returns no step 106 for processing another sample. If available, and the processing steps are repeated.

Alternative Implementations

[0123] Details regarding a related implementation may be found in U.S. Patent 6,142,681 entitled "Method and Apparatus for Interpreting Hybridized Bioelectronic DNA Microarray Patterns Using Self Scaling Convergent Reverberant Dynamics".

[0124] The exemplary embodiments have been primarily described with reference to flow charts illustrating pertinent features of the embodiments. Each method step also represents a hardware or software component for performing the corresponding step. These components are also referred to software component for performing the corresponding step. These components are also referred to herein as a "means for" performing the step. It should be appreciated that not all components of a complete implementation of a practical system are necessarily illustrated or described in detail. Rather, only those components necessary for a thorough understanding of the invention have been illustrated and described in detail. Actual implementations may contain more components or, depending upon the implementation, may contain fewer components.

Claims

1. A method for determining the effectiveness of a therapy by analyzing microarray output patterns generated from biological samples taken at different sampling times from a patient undergoing the therapy, said method comprising the steps of:
5
generating a viral diffusion curve associated with a therapy of interest;
mapping each of the output patterns representative of hybridization activity to respective coordinates on the viral diffusion curve using fractal filtering;
10
determining a degree of convergence between the mapped coordinates on the viral diffusion curves; and
determining whether the therapy of interest has been effective based upon the degree of convergence from one sample to another.
2. The method of claim 1 wherein the step of generating the viral diffusion curve includes the steps of
15
inputting parameters representative of viral load studies for the therapy of interest;
generating a preliminary viral diffusion curve based upon the viral load studies; and
calibrating a degree of directional causality in the preliminary viral diffusion curve to yield the viral diffusion curve.
- 20
3. The method of claim 2 wherein the parameters representative of the viral load studies include one or more of baseline viral load (BVL) set point measurements at which detection is achieved, BVL at which therapy is recommended and viral load markers at which dosage therapy is recommended.
4. The method of claim 2 wherein the step of generating a preliminary viral diffusion curve is performed by:
25
selecting an equation representative of the viral diffusion curve;
determining expectation and mean response parameters for use in parameterizing the equation selected to represent the viral diffusion curve; and
parameterizing the equation selected to represent the viral diffusion curve to yield the preliminary viral diffusion curve.
30
5. The method of claim 4 wherein the step of determining expectation and mean response parameters for use in parameterizing the equation selected to represent the viral diffusion curve comprises the steps of:
35
performing PCR amplification;
obtaining calibrated viral counts from the PCR amplification;
determining the enhanced and normalized hybridization amplitude mean and variance values corresponding to the calibrated viral counts; and
40
matching the enhanced and normalized hybridization amplitude mean and variance values to yield the expectation and mean response parameters.
6. The method of claim 2 wherein the step of calibrating a degree of directional causality in the preliminary viral diffusion curve to yield the viral diffusion curve employs nonlinear information filtering.
- 45
7. The method of claim 1 wherein the step of mapping each output pattern to the viral diffusion curve using fractal filtering comprises the steps of:
generating a partitioned iterated fractal system IFS model representative of the output pattern;
determining affine parameters for IFS model; and
50
mapping the output pattern onto the viral diffusion curve using the IFS.
8. The method of claim 1 wherein the step of determining whether the therapy of interest has been effective includes the steps of:
55
evaluating the degree of convergence against a predetermined threshold of convergence;
if the degree of convergence does not exceed the predetermined threshold, outputting a signal indicating that the therapy of interest has been effective; and
if the degree of convergence exceeds the predetermined threshold, indicating a lack of effectiveness of the

EP 1 145 177 B1

therapy, then performing viral diffusion curve scale matching on the filtered viral diffusion curve and then evaluating whether a predetermined effectiveness time scale has been exceeded, and
if the time scale has been exceeded, outputting a signal indicating the therapy has not been effective, and
if the time scale has not been exceeded, then obtaining a new sample and repeating all steps using the previously generated viral diffusion curve.

9. The method of claim 1 further including the step of compensating for uncertainty in the filtered viral diffusion curves.

10. The method of claim 9 wherein the step of compensating for uncertainty in the filtered viral diffusion curves is performed using non-linear information filtering.

11. The method of claim 1 further including the step, performed before the mapping step, of enhancing the output pattern interferometrically.

12. The method of claim 11 wherein the step of enhancing the output pattern interferometrically comprises the step of performing a nucleic acid amplification.

13. The method of claim 1 wherein the output pattern is a quantized output pattern.

14. The method of claim 13 wherein the quantized output pattern is a dot spectrogram.

15. The method of claim 1 wherein the biological sample is selected from a group consisting of a DNA, RNA, protein, peptide-nucleic acid (PNA) and targeted nucleic amplification (TNA) samples.

16. A system for determining the effectiveness of a therapy by analyzing microarray output patterns generated from biological samples taken at different sampling times from a patient undergoing the therapy, said system comprising:

a viral diffusion curve generator for generating a viral diffusion curve associated with a therapy of interest;
a mapping unit for mapping each of the output patterns representative of hybridization activity to respective coordinates on the viral diffusion curve using fractal filtering;
convergence determination unit for determining a degree of convergence between the mapped coordinates on the viral diffusion curves for determining whether the therapy of interest has been effective based upon the degree of convergence from one sample to another.

17. The system of claim 16 wherein the viral diffusion curve generator includes
an input unit for inputting parameters representative of viral load studies for the therapy of interest;
a preliminary viral diffusion curve generator for generating a preliminary viral diffusion curve based upon the viral load studies; and
a calibration unit for calibrating a degree of directional causality in the preliminary viral diffusion curve to yield the viral diffusion curve.

18. The system of claim 16 wherein the parameters representative of the viral load studies include one or more of baseline viral load (BVL) set point measurements at which detection is achieved, BVL at which therapy is recommended and viral load markers at which dosage therapy is recommended.

19. The method of claim 17 wherein the preliminary viral diffusion curve generator operates by
selecting an equation representative of the viral diffusion curve;
determining expectation and mean response parameters for use in parameterizing the equation selected to represent the viral diffusion curve; and
parameterizing the equation selected to represent the viral diffusion curve to yield the preliminary viral diffusion curve.

20. The system of claim 19 wherein the preliminary viral diffusion curve generator operates to determine expectation and mean response parameters for use in parameterizing the equation selected to represent the viral diffusion curve by:

performing PCR amplification;
obtaining calibrated viral counts from the PCR amplification;

EP 1 145 177 B1

determining the enhanced and normalized hybridization amplitude mean and variance values corresponding to the calibrated viral counts; and
matching the enhanced and normalized hybridization amplitude mean and variance values to yield the expectation and mean response parameters.

5

21. The system of claim 17 wherein the calibration unit employs nonlinear information filtering.

22. The system of claim 16 wherein the mapping unit operates by:

10

generating a partitioned iterated fractal system IFS model representative of the output pattern;
determining affine parameters for IFS model; and
mapping the output pattern onto the viral diffusion curve using the IFS.

23. The system of claim 16 wherein the convergence determination unit operates by:

15

evaluating the degree of convergence against a predetermined threshold of convergence;
if the degree of convergence does not exceed the predetermined threshold, outputting a signal indicating that the therapy of interest has been effective; and
if the degree of convergence exceeds the predetermined threshold, for indicating a lack of effectiveness of the therapy and for performing viral diffusion curve scale matching on the filtered viral diffusion curve and then evaluating whether a predetermined effectiveness time scale has been exceeded, and
if the time scale has been exceeded, outputting a signal indicating the therapy has not been effective, and
if the time scale has not been exceeded, obtaining a new sample and repeating all steps using the previously generated viral diffusion curve.

20

25

24. The system of claim 16 further including a compensation unit for compensating for uncertainty in the filtered viral diffusion curves.

25. The system of claim 24 wherein the compensation unit employs non-linear information filtering.

30

26. The system of claim 16 further including an interferometric enhancement unit for enhancing the output pattern interferometrically.

27. The system of claim 26 wherein the interferometric enhancement unit operates to perform a nucleic acid amplification.

35

28. The system of claim 26 wherein the output pattern is a quantized output pattern.

29. The system of claim 28 wherein the quantized output pattern is a dot spectrogram.

40

30. The system of claim 26 wherein the biological sample is selected from a group consisting of a DNA, RNA, protein, peptide-nucleic acid (PNA) and targeted nucleic amplification (TNA) samples.

31. The method according to one of the claims 1 to 15 wherein output patterns of a biochip are used as the microarray output patterns.

45

32. The system according to one of the claims 16 to 30 for analyzing output patterns of a biochip as the microarray output patterns.

50

Patentansprüche

1. Verfahren zum Ermitteln der Wirksamkeit einer Therapie durch Analyse von aus zu unterschiedlichen Probeentnahmezeitpunkten von einem der Therapie unterzogenen Patienten entnommenen biologischen Proben erzeugten Mikroarrayausgabemustern, wobei das Verfahren die Schritte umfasst:

55

- Erzeugen einer einer im Interesse stehenden Therapie zugeordneten Virusediffusionskurve,
- Abbilden jedes der Hybridisierungsaktivität angegebenden Ausgabemuster auf entsprechende Koordinaten auf

EP 1 145 177 B1

der Virusediffusionskurve unter Verwendung fraktaler Filterung,

- Ermitteln eines Konvergenzgrads zwischen den abgebildeten Koordinaten auf den Virusediffusionskurven, und
- Ermitteln, ob die im Interesse stehende Therapie wirksam war, basierend auf dem Konvergenzgrad von einer Probe zu einer Anderen.

5

2. Verfahren nach Anspruch 1, bei dem der Schritt, die Virusediffusionskurve zu erzeugen, die Schritte aufweist:

- Eingeben von Parametern, die Virusbelastungsstudien für die im Interesse stehende Therapie angeben,
- Erzeugen einer vorläufigen Virusediffusionskurve basierend auf den Virusbelastungsstudien, und
- Kalibrieren eines richtungsabhängigen Kausalitätsgrads in der vorläufigen Virusediffusionskurve, um die Virusediffusionskurve zu erhalten.

10

3. Verfahren nach Anspruch 2, bei dem die die Virusbelastungsstudien angegebenden Parameter von Basislinienvirusbelastungs-(BVL)-Sollwertmessungen, bei denen Detektion erreicht wird, BVL, bei der Therapie empfohlen wird, und Virusbelastungsmarkern, bei denen Dosistherapie empfohlen wird, einen oder mehr aufweisen.

15

4. Verfahren nach Anspruch 2, bei dem der Schritt, eine vorläufige Virusediffusionskurve zu erzeugen, durchgeführt wird durch:

- Wählen einer die Virusediffusionskurve angegebenden Gleichung,
- Ermitteln von Erwartungs- und mittleren Antwortparametern zur Verwendung beim Parametrisieren der zur Angabe der Virusediffusionskurve gewählten Gleichung und
- Parametrisieren der zur Angabe der Virusediffusionskurve gewählten Gleichung, um die vorläufige Virusediffusionskurve zu erhalten.

20

25

5. Verfahren nach Anspruch 4, bei dem der Schritt, Erwartungs- und mittlere Antwortparameter zur Verwendung beim Parametrisieren der zur Angabe der Virusediffusionskurve gewählten Gleichung zu ermitteln, die Schritte umfasst:

- Durchführen einer PCR-Verstärkung,
- Erhalten von kalibrierten Viruszahlungen aus der PCR-Verstärkung,
- Ermitteln der den kalibrierten Viruszahlungen entsprechenden Mittel- und Varianzwerten der verstärkten und normalisierten Hybridisierungsamplituden, und
- Abgleichen der Mittel- und Varianzwerte der verstärkten und normalisierten Hybridisierungsamplituden, um die Erwartungs- und mittleren Antwortparameter zu erhalten.

30

35

6. Verfahren nach Anspruch 2, bei dem der Schritt, einen richtungsabhängigen Kausalitätsgrad in der vorläufigen Virusediffusionskurve zu kalibrieren, um die Virusediffusionskurve zu erhalten, nicht lineare Informationsfilterung verwendet.

40

7. Verfahren nach Anspruch 1, bei dem der Schritt, jedes Ausgabemuster auf die Virusediffusionskurve unter Verwendung fraktaler Filterung abzubilden, die Schritte umfasst:

- Erzeugen eines das Ausgabemuster angegebenden, partitionierten iterierten Fraktalsystem-IFS-Modell,
- Ermitteln affiner Parameter für das IFS-Modell, und
- Abbilden des Ausgabemusters auf die Virusediffusionskurve unter Verwendung des IFS.

45

8. Verfahren nach Anspruch 1, bei dem der Schritt, zu Ermitteln, ob die im Interesse stehende Therapie wirksam war, die Schritte aufweist:

- Evaluieren des Konvergenzgrads gegenüber einem vorbestimmten Konvergenzgrenzwert,
- Ausgeben eines Signals, das angibt, dass die im Interesse stehende Therapie wirksam war, wenn der Konvergenzgrad den vorbestimmten Grenzwert nicht überschreitet, und
- Angeben eines Fehlens der Wirksamkeit der Therapie, wenn der Konvergenzgrad den vorbestimmten Grenzwert überschreitet, wobei dann eine Skalierungsanpassung der Virusediffusionskurve auf die gefilterte Virusediffusionskurve durchgeführt und dann evaluiert wird, ob ein vorbestimmter Wirksamkeitszeitmaßstab überschritten wurde, und
- Ausgeben eines Signals, das angibt, dass die Therapie nicht wirksam war, wenn der Zeitmaßstab überschritten wurde, und

50

55

EP 1 145 177 B1

- Erhalten einer neuen Probe und Wiederholen aller Schritte unter Verwendung der zuvor erzeugten Virusdiffusionskurve dann, wenn der Zeitmaßstab nicht überschritten wurde.
- 5 9. Verfahren nach Anspruch 1, ferner den Schritt aufweisend, Unschärfen in den gefilterten Virusdiffusionskurven zu kompensieren.
10. Verfahren nach Anspruch 9, bei dem der Schritt, Unschärfen in den gefilterten Virusdiffusionskurven zu kompensieren, unter Verwendung nicht linearer Informationsfilterung durchgeführt wird.
- 10 11. Verfahren nach Anspruch 1, ferner den vor dem Abbildungsschritt durchgeführten Schritt aufweisend, das Ausgabemuster interferometrisch zu verstärken.
12. Verfahren nach Anspruch 11, bei dem der Schritt, das Ausgabemuster interferometrisch zu verstärken, den Schritt umfasst, eine Nukleinsäureverstärkung durchzuführen.
- 15 13. Verfahren nach Anspruch 1, bei dem das Ausgabemuster ein quantisiertes Ausgabemuster ist.
14. Verfahren nach Anspruch 13, bei dem das quantisierte Ausgabemuster ein Punktspektrogramm ist.
- 20 15. Verfahren nach Anspruch 1, bei dem die biologische Probe aus einer Gruppe ausgewählt wird, die aus DNA-, RNA-, Protein-, Peptid-Nukleinsäure-(PNA)- und Target-Nukleidverstärkungs-(TNA)-Proben besteht.
- 25 16. System zum Ermitteln der Wirksamkeit einer Therapie durch Analyse von aus zu unterschiedlichen Probenentnahmezeitpunkten von einem der Therapie unterzogenen Patienten erhaltenen biologischen Proben erzeugten Mikroarrayausgabemustern, wobei das System umfasst:
- einen Virusdiffusionskurvengenerator zum Erzeugen einer einer im Interesse stehenden Therapie zugeordneten Virusdiffusionskurve,
 - eine Abbildungseinheit zum Abbilden jedes der Hybridisierungsaktivität angegebenden Ausgabemuster auf entsprechende Koordinaten auf der Virusdiffusionskurve unter Verwendung fraktaler Filterung,
 - einer Konvergenzermittlungseinheit zum Ermitteln eines Konvergenzgrads zwischen den abgebildeten Koordinaten auf den Virusdiffusionskurven, um zu ermitteln, ob die im Interesse stehende Therapie wirksam war, basierend auf dem Konvergenzgrad von einer Probe zu einer Anderen.
- 30 17. System nach Anspruch 16, bei dem der Virusdiffusionskurvengenerator aufweist:
- eine Eingabeeinheit zum Eingeben von Parametern, die Virusbelastungsstudien über die im Interesse stehende Therapie angeben,
 - einen Generator für eine vorläufige Virusdiffusionskurve, um eine vorläufige Virusdiffusionskurve basierend auf den Virusbelastungsstudien zu erzeugen, und
 - eine Kalibrierungseinheit zum Kalibrieren eines richtungsabhängigen Kausalitätsgrads in der vorläufigen Virusdiffusionskurve, um die Virusdiffusionskurve zu erhalten.
- 35 18. System nach Anspruch 16, bei dem die die Virusbelastungsstudien angegebenden Parameter von Basislinienvirusbelastungs-(BVL)-Sollwertmessungen, bei denen Detektion erreicht wird, BVL, bei der Therapie empfohlen wird, und Virusbelastungsmarkern, bei dem eine Dosistherapie empfohlen wird, eine oder mehr aufweisen.
- 40 19. Verfahren nach Anspruch 17, bei dem der Generator für eine vorläufige Virusdiffusionskurve arbeitet durch:
- Wählen einer die Virusdiffusionskurve angegebenden Gleichung,
 - Ermitteln von Erwartungs- und mittleren Antwortparametern zur Verwendung beim Parametrisieren der zur Angabe der Virusdiffusionskurve gewählten Gleichung, und
 - Parametrisieren der zur Angabe der Virusdiffusionskurve gewählten Gleichung, um die vorläufige Virusdiffusionskurve zu erhalten.
- 45 20. System nach Anspruch 19, bei dem der Generator für eine vorläufige Virusdiffusionskurve zum Ermitteln von Erwartungs- und mittleren Antwortparametern zur Verwendung beim Parametrisieren der zur Angabe der Virusdiffusionskurve gewählten Gleichung arbeitet durch:
- 50
- 55

EP 1 145 177 B1

- Durchführen einer PCR-Verstärkung,
- Erhalten kalibrierter Viruszahlungen aus der PCR-Verstärkung,
- Ermitteln der den kalibrierten Viruszahlungen entsprechenden Mittel- und Varianzwerten der verstärkten und normalisierten Hybridisierungsamplituden, und
- 5 - Abgleichen der Mittel- und Varianzwerte der verstärkten und normalisierten Hybridisierungsamplituden, um die Erwartungs- und mittleren Antwortparameter zu erhalten.

21. System nach Anspruch 17, bei die Kalibrierungseinheit nicht lineare Informationsfilterung verwendet.

10 22. System nach Anspruch 16, bei dem die Abbildungseinheit arbeitet durch:

- Erzeugen eines das Ausgabemuster angehenden, partitionierten iterierten Fraktalsystem-IFS-Modells,
- Ermitteln affiner Parameter für das IFS-Modell, und
- Abbilden des Ausgabemusters auf die Virusdiffusionskurve unter Verwendung des IFS.

15 23. System nach Anspruch 16, bei dem die Konvergenzermittlungseinheit arbeitet durch:

- Evaluieren des Konvergenzgrades gegenüber einem vorbestimmten Konvergenzgrenzwert,
- 20 - Ausgeben eines Signals, das angibt, dass die im Interesse stehende Therapie wirksam war, wenn der Konvergenzgrad den vorbestimmten Grenzwert nicht überschreitet, und
- Angeben eines Fehlens der Wirksamkeit der Therapie und Durchführen einer Skalierungsanpassung der Virusdiffusionskurve an die gefilterte Virusdiffusionskurve und dann Evaluieren, ob ein vorbestimmter Wirksamkeitszeitmaßstab überschritten wurde, wenn der Konvergenzgrad den vorbestimmten Grenzwert überschreitet, und
- 25 - Ausgeben eines Signals, das angibt, dass die Therapie nicht wirksam war, wenn der Zeitmaßstab überschritten wurde, und
- Erhalten einer neuen Probe und Wiederholen aller Schritte unter Verwendung der zuvor erzeugten Virusdiffusionskurve, wenn der Zeitmaßstab nicht überschritten wurde.

30 24. System nach Anspruch 16, ferner mit einer Kompensationseinheit, um Unschärfen in den gefilterten Virusdiffusionskurven zu kompensieren.

25. System nach Anspruch 24, bei dem die Kompensationseinheit nicht lineare Informationsfilterung verwendet.

35 26. System nach Anspruch 16, ferner mit einer interferometrischen Verstärkungseinheit, um das Ausgabemuster interferometrisch zu verstärken.

27. System nach Anspruch 26, bei dem die interferometrische Verstärkungseinheit arbeitet, um eine Nukleidsäureverstärkung durchzuführen.

40 28. System nach Anspruch 26, bei dem das Ausgabemuster ein quantisiertes Ausgabemuster ist.

29. System nach Anspruch 28, bei dem das quantisierte Ausgabemuster ein Punktspektrogramm ist.

45 30. System nach Anspruch 26, bei dem die biologische Probe von einer Gruppe ausgewählt ist, die aus DNA-, RNA-, Protein-, Peptid-Nukleidsäure-(PNA)- und Targetnucleidverstärkungs-(TNA)-Proben besteht.

31. Verfahren nach einem der Ansprüche 1 bis 15, bei dem Ausgabemuster eines Biochips als die Mikroarrayausgabemuster verwendet werden.

50 32. System nach einem der Ansprüche 16 bis 30, um Ausgabemuster eines Biochips als die Mikroarrayausgabemuster zu analysieren.

55 Revendications

1. Procédé de détermination de l'efficacité d'une thérapie par analyse de modèles de résultats de micro-dépôts générés à partir d'échantillons biologiques prélevés à différents points d'échantillonnage chez un patient recevant

EP 1 145 177 B1

cette thérapie, ledit procédé comprenant les étapes consistant à :

généraliser une courbe de diffusion virale associée à la thérapie concernée ;
cartographier, sous forme de coordonnées respectives, chacun des modèles de résultats représentatifs de
l'activité d'hybridisation sur la courbe de diffusion virale à l'aide d'une technique de filtration fractale ;
déterminer un degré de convergence entre les coordonnées respectives des différents modèles de résultats
cartographiés sur les courbes de diffusion virale ; et
déterminer l'efficacité de la thérapie concernée d'après le degré de convergence d'un échantillon à un autre.

2. Procédé selon la revendication 1, dans lequel l'étape consistant à généraliser la courbe de diffusion virale inclut les étapes consistant à :

entrer les paramètres représentatifs d'études de charge virale pour la thérapie concernée ;
généraliser une courbe de diffusion virale préliminaire sur la base des études de charge virale ; et
calibrer un degré de causalité directionnelle à partir de la courbe de diffusion virale préliminaire pour donner
la courbe de diffusion virale.

3. Procédé selon la revendication 2, dans lequel les paramètres représentatifs des études de charge virale incluent un ou plusieurs points de mesure prédéfinis de la charge virale de base (CVB) auxquels la détection est possible, CVB à laquelle la thérapie est recommandée et marqueurs que constitue la charge virale aux quantités desquels la thérapie est recommandée.

4. Procédé selon la revendication 2, dans lequel l'étape consistant à généraliser une courbe de diffusion virale est conduite en :

choisissant une équation représentative de la courbe de diffusion virale ;
déterminant des paramètres de valeur attendue et de réponse moyenne utilisés dans le paramétrage de l'équation choisie pour représenter la courbe de diffusion virale ; et
paramétrant l'équation choisie pour représenter la courbe de diffusion virale afin de donner la courbe de diffusion virale préliminaire.

5. Procédé selon la revendication 4, dans lequel l'étape consistant à déterminer des paramètres de valeur attendue et de réponse moyenne utilisés dans le paramétrage de l'équation choisie pour représenter la courbe de diffusion virale comprend les étapes consistant à :

procéder à une amplification par PCR ;
obtenir une quantité de virus calibrée à partir de l'amplification par PCR ;
déterminer les valeurs de moyenne et de variance de l'hybridisation accrue et normalisée correspondant à la quantité de virus ; et
harmoniser les valeurs de moyenne et de variance de l'hybridisation accrue et normalisée correspondant à la quantité de virus pour donner les paramètres de valeur attendue et de réponse moyenne.

6. Procédé selon la revendication 2, dans lequel l'étape consistant à calibrer un degré de causalité directionnelle à partir de la courbe de diffusion virale préliminaire pour donner la courbe de diffusion virale utilise une technique de filtration de l'information non linéaire.

7. Procédé selon la revendication 1, dans lequel l'étape consistant à cartographier chacun des modèles de résultats sur la courbe de diffusion virale à l'aide d'une technique de filtration fractale comprend les étapes consistant à :

généraliser un modèle de système fractal itéré (IFS) partitionné représentatif du modèle de résultat ;
déterminer des paramètres affins pour le modèle IFS ; et
cartographier le modèle de résultat par dessus la courbe de diffusion virale à l'aide du modèle IFS.

8. Procédé selon la revendication 1, dans lequel l'étape consistant à déterminer l'efficacité de la thérapie concernée comprend les étapes consistant à :

évaluer le degré de convergence par rapport à un seuil de convergence prédéterminé ;
si le degré de convergence ne dépasse pas le seuil prédéterminé, produire un signal indiquant que la thérapie

EP 1 145 177 B1

concernée est efficace ; et
si le degré de convergence dépasse le seuil prédéterminé, indiquer le manque d'efficacité de la thérapie, puis harmoniser l'échelle de la courbe de diffusion virale d'après la courbe de diffusion virale filtrée et déterminer si l'échelle de temps d'efficacité prédéterminée est dépassée ; et
si l'échelle de temps est dépassée, produire un signal indiquant que la thérapie n'est pas efficace, et
si l'échelle de temps n'est pas dépassée, obtenir alors un nouvel échantillon et répéter toutes les étapes à l'aide de la courbe de diffusion virale précédemment générée.

9. Procédé selon la revendication 1 incluant en outre l'étape consistant à compenser l'incertitude associée aux courbes de diffusion virale filtrées.

10. Procédé selon la revendication 9, dans lequel l'étape consistant à compenser l'incertitude associée aux courbes de diffusion virale filtrées est conduite à l'aide d'une technique de filtration de l'information non linéaire.

11. Procédé selon la revendication 1 incluant en outre l'étape consistant à accroître le modèle de résultat interférométriquement, conduite avant l'étape de cartographie.

12. Procédé selon la revendication 11, dans lequel l'étape consistant à accroître le modèle de résultat interférométriquement comprend l'étape d'amplification d'acides nucléiques.

13. Procédé selon la revendication 1, dans lequel le modèle de résultat est un modèle de résultat quantifié.

14. Procédé selon la revendication 13, dans lequel le modèle de résultat quantifié est un spectrogramme matriciel.

15. Procédé selon la revendication 1, dans lequel l'échantillon biologique est choisi parmi un groupe consistant en ADN, ARN, une protéine, un acide peptide nucléaire (APN) et des échantillons d'amplification nucléaire ciblée (ANC).

16. Système de détermination de l'efficacité d'une thérapie par analyse de modèles de résultats de micro-dépôts générés à partir d'échantillons biologiques prélevés à différents points d'échantillonnage chez un patient recevant cette thérapie, ledit système comprenant :

un générateur de courbe de diffusion virale permettant de générer une courbe de diffusion virale associée à la thérapie concernée ;

une unité de cartographie permettant de cartographier, sous forme de coordonnées respectives, chacun des modèles de résultats représentatifs de l'activité d'hybridisation sur la courbe de diffusion virale à l'aide d'une technique de filtration fractale ;

une unité de détermination de la convergence permettant de déterminer un degré de convergence entre les coordonnées respectives des différents modèles de résultats cartographiés sur les courbes de diffusion virale afin de déterminer l'efficacité de la thérapie concernée d'après le degré de convergence d'un échantillon à un autre.

17. Système selon la revendication 16, dans lequel le générateur de courbe de diffusion virale inclut une unité d'entrée permettant d'entrer les paramètres représentatifs des études de charge virale pour la thérapie concernée ;

un générateur de courbe de diffusion virale préliminaire permettant de générer une courbe de diffusion virale préliminaire d'après les études de charge virale ; et

une unité de calibrage permettant de calibrer un degré de causalité directionnelle à partir de la courbe de diffusion virale préliminaire pour donner la courbe de diffusion virale.

18. Système selon la revendication 16, dans lequel les paramètres représentatifs des études de charge virale incluent un ou plusieurs points de mesure prédéfinis de la charge virale de base (CVB) auxquels la détection est possible, CVB à laquelle la thérapie est recommandée et marqueurs que constitue la charge virale aux quantités desquels la thérapie est recommandée.

19. Procédé selon la revendication 17, dans lequel le générateur de courbe de diffusion virale préliminaire opère en :

choisissant une équation représentative de la courbe de diffusion virale ;

EP 1 145 177 B1

déterminant des paramètres de valeur attendue et de réponse moyenne utilisés dans le paramétrage de l'équation choisie pour représenter la courbe de diffusion virale ; et paramétrant l'équation choisie pour représenter la courbe de diffusion virale afin de donner la courbe de diffusion virale préliminaire.

5

20. Système selon la revendication 19, dans lequel le générateur de courbe de diffusion virale préliminaire détermine les paramètres de valeur attendue et de réponse moyenne utilisés dans le paramétrage de l'équation choisie pour représenter la courbe de diffusion virale en :

10

procédant à une amplification par PCR ;
obtenant une quantité de virus calibrée à partir de l'amplification par PCR ;
déterminant les valeurs de moyenne et de variance de l'hybridisation normalisée et accrue correspondant à la quantité de virus ; et
harmonisant les valeurs de moyenne et de variance de l'hybridisation accrue et normalisée correspondant à la quantité de virus pour donner les paramètres de valeur attendue et de réponse moyenne.

15

21. Système selon la revendication 17, dans lequel l'unité de calibrage utilise une technique de filtration de l'information non linéaire.

20

22. Système selon la revendication 16, dans lequel l'unité de cartographie opère en :

généralisant un modèle de système fractal itéré (IFS) partitionné représentatif du modèle de résultat ;
déterminant des paramètres affins pour le modèle IFS ; et
cartographiant le modèle de résultat par dessus la courbe de diffusion virale à l'aide
du modèle IFS.

25

23. Système selon la revendication 16, dans lequel l'unité de détermination de la convergence opère en :

évaluant le degré de convergence par rapport à un seuil de convergence prédéterminé ;
si le degré de convergence ne dépasse pas le seuil prédéterminé, en produisant un signal indiquant que la
thérapie concernée est efficace ; et
si le degré de convergence dépasse le seuil prédéterminé, en indiquant un manque d'efficacité de la thérapie,
puis en harmonisant l'échelle de la courbe de diffusion virale d'après la courbe de diffusion virale filtrée et en
déterminant si l'échelle de temps d'efficacité prédéterminée est dépassée ; et
si l'échelle de temps est dépassée, en produisant un signal indiquant que la thérapie concernée n'est pas
efficace ; et
si l'échelle de temps n'est pas dépassée, en obtenant alors un nouvel échantillon et en répétant toutes les
étapes à l'aide de la courbe de diffusion virale précédemment générée.

30

35

40

24. Système selon la revendication 16 incluant en outre une unité de compensation de l'incertitude associée aux courbes de diffusion virale filtrées.

25. Système selon la revendication 24, dans lequel l'unité de compensation utilise une technique de filtration de l'information non linéaire.

45

26. Système selon la revendication 16 incluant en outre une unité d'accroissement interférométrique permettant d'accroître le modèle de résultat interférométriquement.

50

27. Système selon la revendication 26, dans lequel le fonctionnement de l'unité d'accroissement interférométrique comprend l'amplification d'acides nucléiques.

28. Système selon la revendication 26, dans lequel le modèle de résultat est un modèle de résultat quantifié.

29. Système selon la revendication 28, dans lequel le modèle de résultat quantifié est un spectrogramme matriciel.

55

30. Système selon la revendication 26, dans lequel l'échantillon biologique est choisi parmi un groupe consistant en ADN, ARN, une protéine, un acide peptide nucléique (APN) et des échantillons d'amplification nucléique ciblée (ANC).

EP 1 145 177 B1

31. Procédé selon l'une quelconque des revendications 1 à 15, dans lequel les modèles de résultats d'une biopuce sont utilisés comme modèles de résultats de micro-dépôts.

5 32. Système d'analyse de modèles de résultats d'une biopuce comme modèles de résultats de micro-dépôts selon l'une quelconque des revendications 16 à 30.

10

15

20

25

30

35

40

45

50

55

FIGURE 1

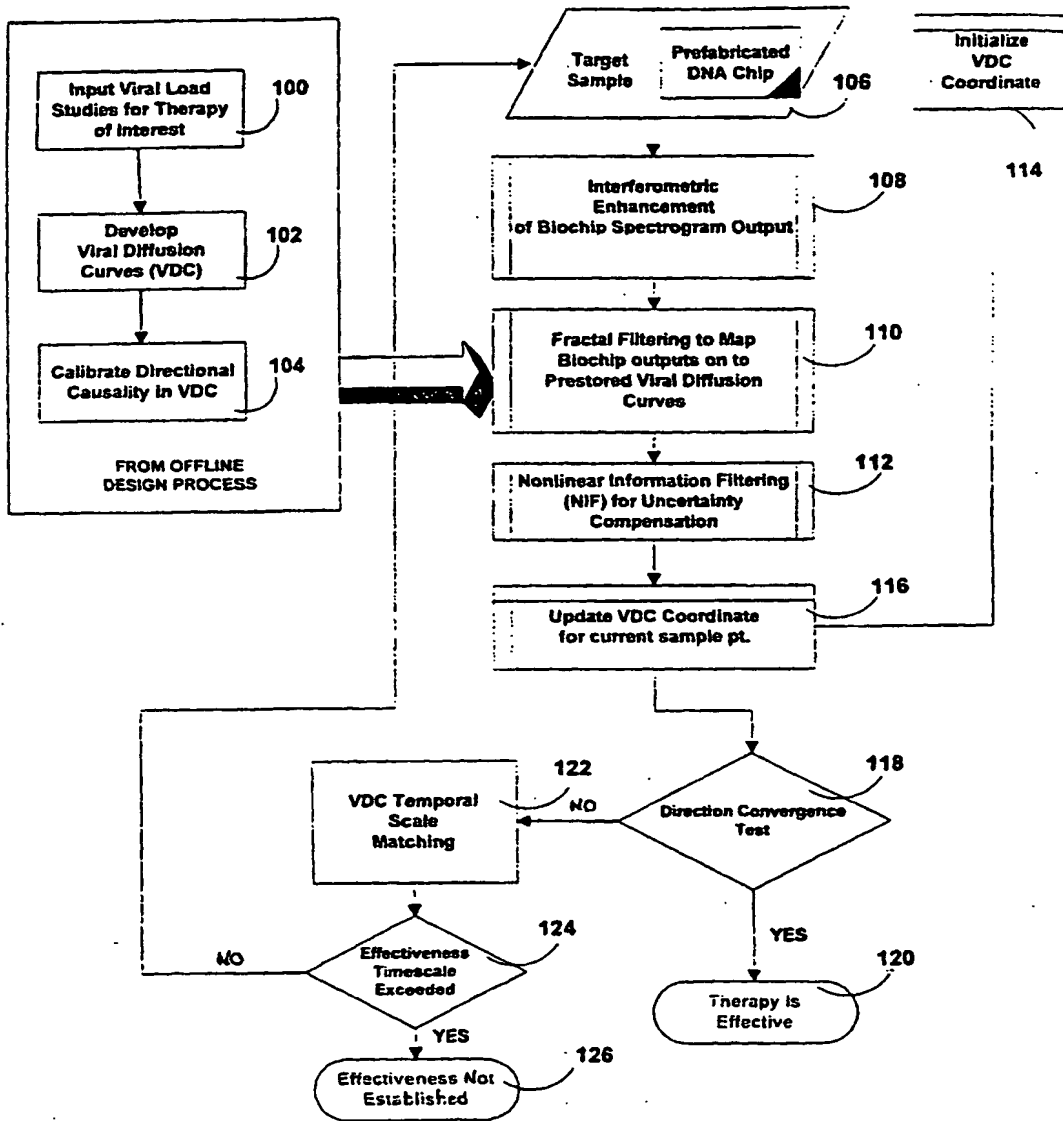


FIGURE 2

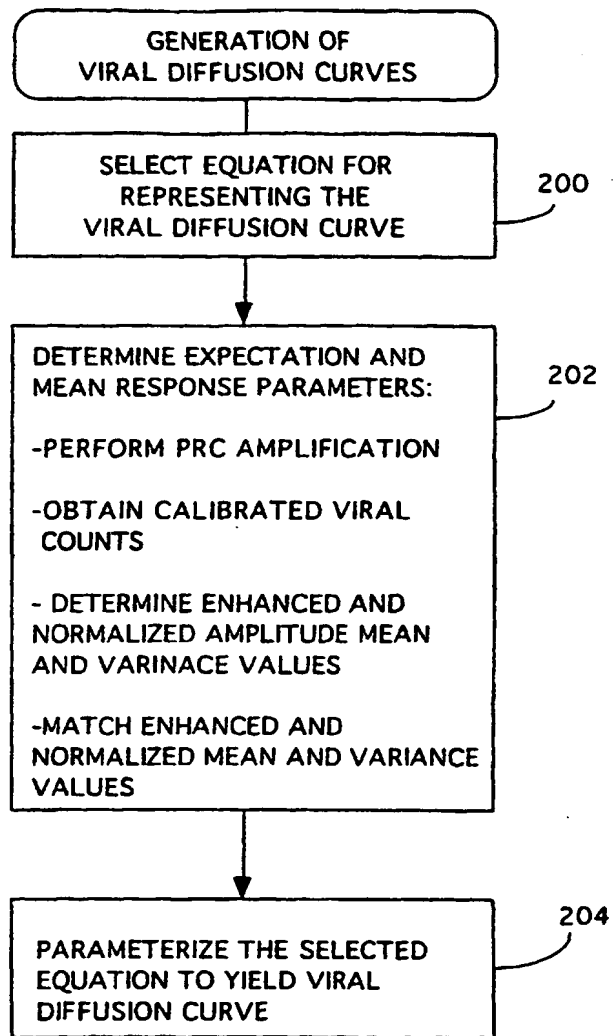
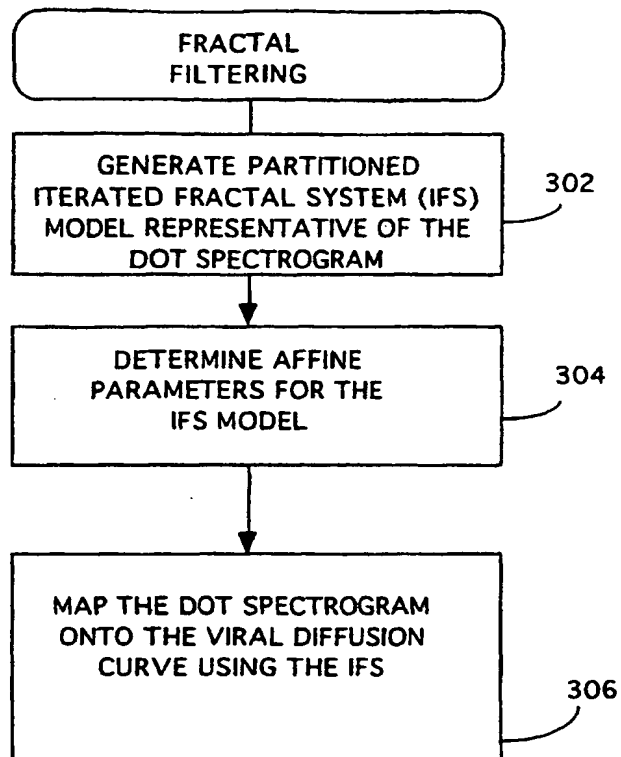


FIGURE 3



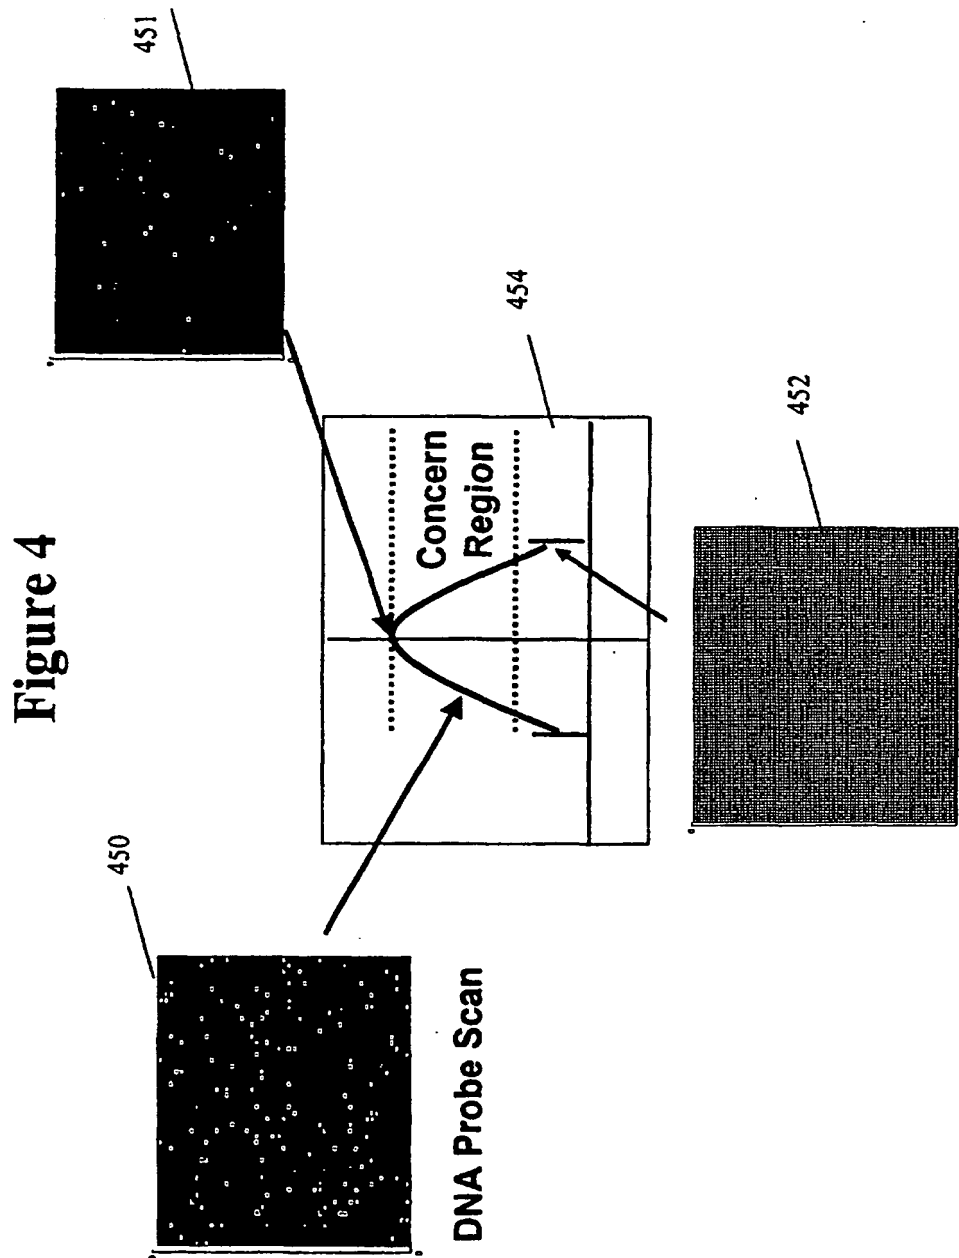


FIGURE 5

